Ministry of Jal Shakti,
Department of Water Resources, River Development and Ganga Rejuvenation,
Government of India

सत्यमेव जयते

जल शक्ति मंत्रालय,
जल संसाधन विभाग,
नदी विकास एवं गंगा संरक्षण विभाग,
भारत सरकार

CENTRAL WATER AND POWER RESEARCH STATION, PUNE - 411 024

DATA LOGGER & TELEMETRY

TEST & CALIBRATE

- ✓Voltage (AC,DC)
- ✓Current (AC,DC)
- ✓Resistance
- ✓Capacitance
- ✓RTD
- ✓Thermocouple
- ✓VSWR
- ✓Impedance Matching
- ✓Distance to fault

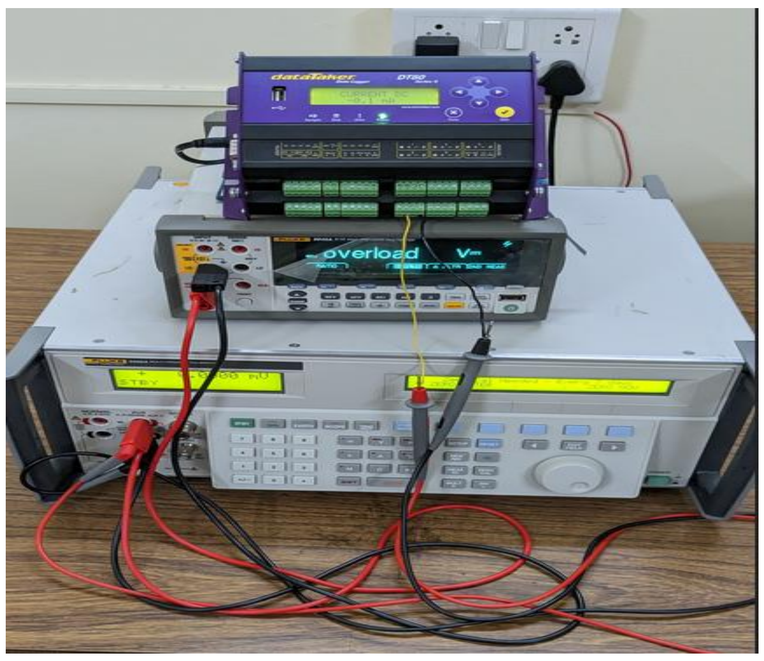

Unique Feature

- Accuracy of 50 ppm for Testing up to 1000 DC
- Frequency range up to 8GHz for RF Cable & Antenna Testing
- Calibration using NIST Standards

Contact: Mrs R S Erande, Scientist-C & In charge Data Logger Testing & Calibration Facility
Shri. P.K.Dorle , Scientist-C & In charge Telemetry Testing & Calibration Facility
Phone: 020 2410 3437/3404
Email: director@cwprs.gov.in / reshmi.kv@gov.in / erande.rs@cwprs.gov.in / dorle.pk@cwprs.gov.in